


STERI-PAK™ LF PACK

Interpretation Guide

Disposable Bowie-Dick Test Pack


Catalog No. BD 111

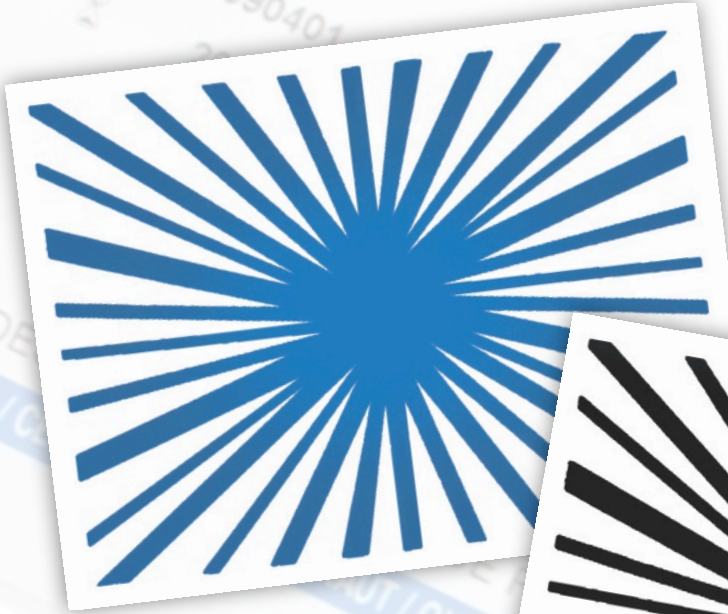

CORRECT COLOR CHANGE

UNEXPOSED

Color change will occur from the center of the card outward. Designed to change color from blue to black when all parameters are met.

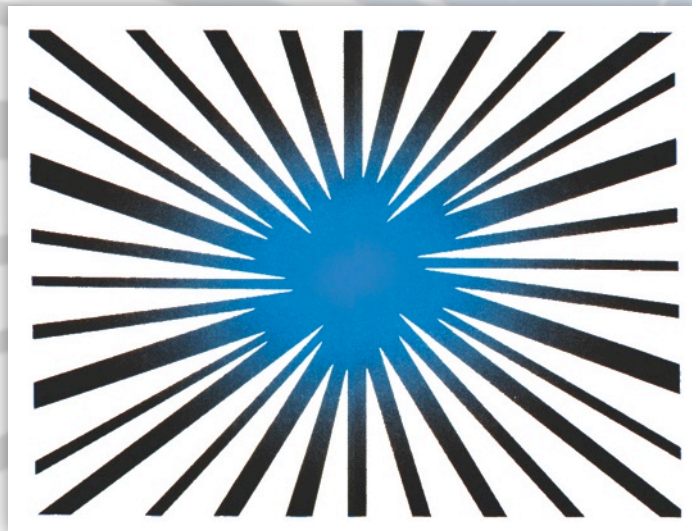

FAIL

If any blue color remains in the center of the card, exposure to sterilization conditions are insufficient